


## The KRONNER SIDE-KICK

### Abbreviated Instructions for Use for holding the **VCare** uterine manipulator

For detailed instructions see the INSTRUCTIONS FOR USE booklet or CD

[Detailed instructions on Kronner.com](http://Kronner.com)

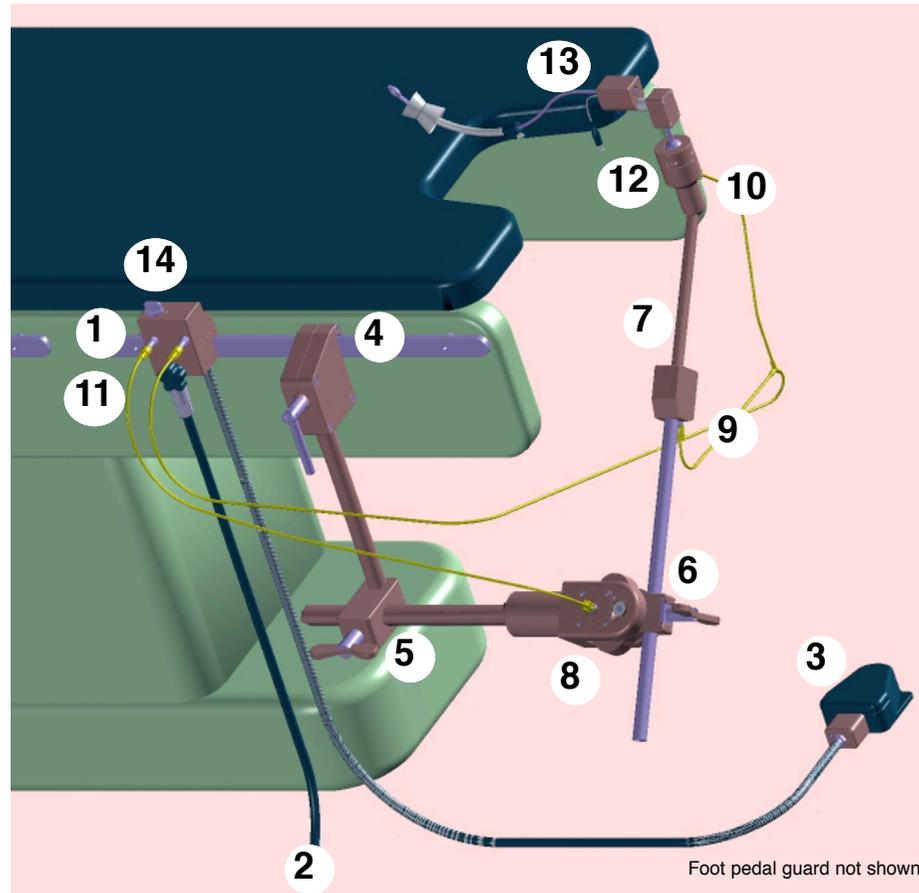


Kronner Medical, 1443 Upper Cleveland Rapids Road, Roseburg, OR 97471  
Tel: 541-672-2543

### Attaching the SideKick assembly to the operating table rail.

1. Attach the gas supply module to the operating table rail and turn off the module switch.
2. Connect the gas supply hose to the hospital nitrogen supply.
3. Position the foot pedal. **Warning: Do not attach a gas line to a uterine manipulator, extreme danger.**
4. Attach the rail grip to the rail.
5. Slide the pivot rod into the rail grip.
6. Insert the outer arm into the pivot.
7. Insert the inner rod into the outer arm.
8. Attach the single gas line to the pivot and the other end to the gas supply module #1.
9. Attach one branch of the branched line to the outer arm luer.
10. Attach the second branch of the branched line to the inner rod ball joint luer.
11. Attach the other end of the branched line to the gas supply module.
12. Attach the adapter to the inner rod.
13. Attach the adapter to the manipulator after insertion of the manipulator into the patient, see VCare instructions below.
14. Turn the gas module switch to "ON".
15. When repositioning the manipulator, step on the foot pedal #3.


### Attaching the adapter to the Inner Rod

1. Connect the adapter to the inner rod by sliding the two adapter notches over the two inner rod pins and rotating the adapter clockwise. Gas pressure must be off during this step.

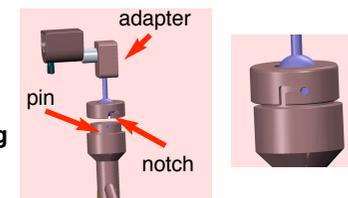

### Attaching the adapter to the V-Care manipulator

1. With the gas off, place the V-care handle grip over the V-care handle.
2. Tighten the joining screw.  
Support the arm until the gas is turned on.

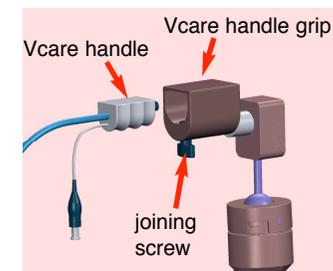

United States Patent 8,485,484.B2