
The KRONNER SIDE-KICK

for holding uterine manipulators

Abbreviated Disassembling Instructions

for detailed instructions see the Instructions for Use booklet or CD

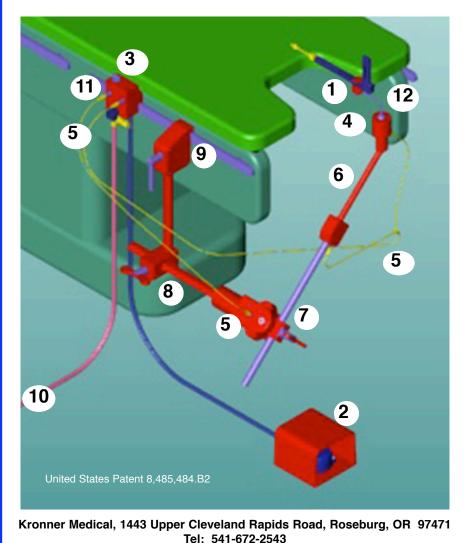

Disassembling SIDEKICK for all manipulators

- 1. Step on the foot pedal and remove the manipulator* from the patient with SideKick attached or detach Sidekick from the manipulator by reversing the assemly instructions.
- 2. Continue stepping on the foot pedal and lower the arm to the stop. **DO NOT FORCE THE STOP.**
- 3. Shut off the gas switch on the gas supply module. This must be done prior to removing the gas lines.
- 4. Disconnect the adapter with or wihout the attached manipulator from the inner rod ball joint.
- 5. Remove the gas lines.
- 6. Remove the inner rod from the outer arm.
- 7. Remove the outer arm from the pivot. **Perform steps 6 & 7 prior to elevating the dropped table section. Dropped table section not shown.**
- 8. Remove the pivot from the rail grip.
- 9. Remove the rail grip from the table rail.
- 10. Detach the gas module supply hose from the wall supply.
- 11. Detach the gas supply module from the table rail.
- 12. If attached, detach the manipulator from the adapter by reversing the assembly instructions.
- *Note: The manipulator shown as an example is the RUMI.